



**For Research Use Only, Not for use in diagnostic procedures**

ELISA Kit for Measuring Human S100A11

# CircuLex S100A11 ELISA Kit

Cat# CY-8063

Intended Use..... 1  
Storage..... 1  
Introduction..... 2  
Principle of the Assay..... 2-3  
Materials Provided..... 3  
Materials Required but not Provided..... 4  
Precautions and Recommendations..... 5  
Sample Collection and Storage..... 6  
Detailed Protocol..... 7-8  
Calculations..... 9  
Measurement Range..... 9  
Troubleshooting..... 9  
Reagent Stability..... 9  
Assay Characteristics..... 10-12  
Example of Test Results..... 13-14  
References..... 15

## Intended Use

The MBL Research Product **CircuLex S100A11 ELISA Kit** is used for the quantitative measurement of human S100A11 in serum and cell culture supernatant.

Individual users should determine appropriate conditions when using other types of samples.

**This assay kit is for research use only and not for use in diagnostic or therapeutic procedures.**

### Storage

- Upon receipt store all components at 4°C.
- Don't expose reagents to excessive light.

---

## Introduction

---

S100A11 is a member of the S100 family of EF-hand Ca<sup>2+</sup>-binding proteins, whose expression is ubiquitous in various tissues including skin, smooth muscle and other tissues at different levels, with a high expression level in the skin. It is also known as calgizzarin (1) and S100C (2). S100A11 was shown to bind to annexin A1 and the S100A11/annexin A1 complex is a heterotetramer consisting of two S100A11 and two annexin A1 proteins. Ca<sup>2+</sup> binding to S100A11 induces a conformational change that exposes a hydrophobic surface for interaction with target proteins (3). In addition to binding to annexin A1, S100A11 has been shown to interact with annexin A6 (4), actin (5) and transglutaminase (6), and is capable of forming a heterodimer with S100B through subunit exchange (7).

It was reported that S100A11, which is actively secreted by NHK (normal human keratinocyte), acts on NHK to enhance the production of EGF family proteins, resulting in growth stimulation (8). On the other hand, inhibitory signals such as TGFβ or high-calcium promote S100A11/annexin A1 to translocate into the nucleus and induce p21/WAF1 resulting in growth inhibition (9). These findings indicate that S100A11 plays a dual role in growth regulation, being suppressive in cells and being promotive from outside of cells. S100A11 seems to act as either a tumor suppressor or promoter in many different types of tumors and would play respective roles in influencing the proliferation of the cancer cells.


---

## Principle of the Assay

---

The MBL Research Product **CircuLex S100A11 ELISA Kit** employs the quantitative sandwich enzyme immunoassay technique. A mouse monoclonal antibody specific for human S100A11 is pre-coated onto a microplate. Standards and samples are pipetted into the wells and the immobilized antibody binds any human S100A11 present. After washing away any unbound substances, an HRP conjugated antibody specific for human S100A11 is added to the wells. Following a wash to remove any unbound antibody HRP conjugate, the remaining conjugate is allowed to react with the substrate H<sub>2</sub>O<sub>2</sub>-tetramethylbenzidine. The reaction is stopped by addition of acidic solution and absorbance of the resulting yellow product is measured at 450 nm. The absorbance is proportional to the concentration of human S100A11. A standard curve is constructed by plotting absorbance values versus human S100A11 concentrations of calibrators, and concentrations of unknown samples are determined using this standard curve.

## Summary of Procedure

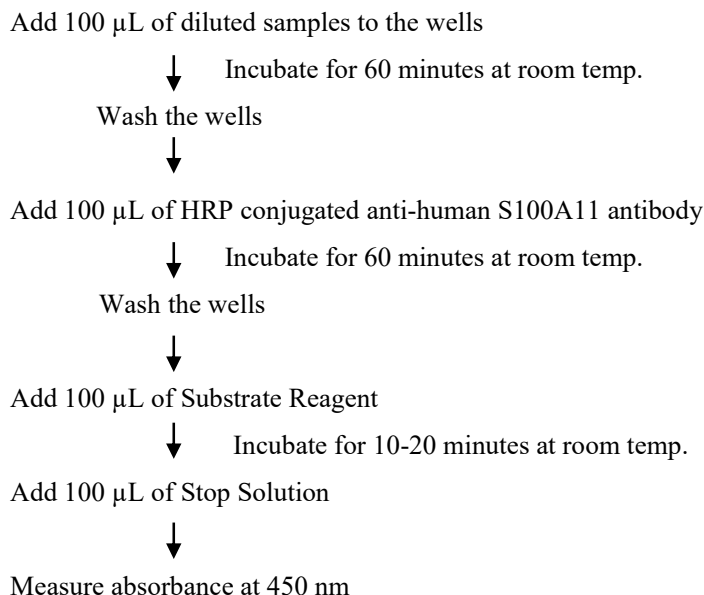

---

## Materials Provided

---

All samples and standards should be assayed in duplicate. The following components are supplied and are sufficient for the one 96-well microplate kit.

**Microplate:** One microplate supplied ready to use, with 96 wells (12 strips of 8-wells) in a foil, zip-lock bag with a desiccant pack. Wells are coated with mouse anti-human S100A11 monoclonal antibody (YK-1A4) as a capture antibody.

**10X Wash Buffer:** One bottle containing 100 mL of 10X buffer containing Tween®-20

**Dilution Buffer:** Two bottles containing 20 mL of 1X buffer; use for sample dilution. Ready to use.

**Human S100A11 Standard:** One vial containing X\* ng of lyophilized recombinant human S100A11  
**\*The amount is changed depending on lot. See the real "User's Manual" included in the kit box.**

**HRP conjugated Detection Antibody:** One bottle containing 12 mL of HRP (horseradish peroxidase) conjugated anti-human S100A11 antibody. Ready to use.

**Substrate Reagent:** One bottle containing 20 mL of the chromogenic substrate, tetra-methylbenzidine (TMB). Ready to use.

**Stop Solution:** One bottle containing 20 mL of 1 N H<sub>2</sub>SO<sub>4</sub>. Ready to use.

---

## Materials Required but not Provided

---

- **Pipettors:** 2-20  $\mu\text{L}$ , 20-200  $\mu\text{L}$  and 200-1,000  $\mu\text{L}$  precision pipettors with disposable tips.
- **Precision repeating pipettor**
- **Orbital microplate shaker**
- **Microcentrifuge and tubes** for sample preparation.
- **Vortex mixer**
- **(Optional) Microplate washer:** Manual washing is possible but not preferable.
- **Plate reader** capable of measuring absorbance in 96-well plates at dual wavelengths of 450 nm/540 nm. Dual wavelengths of 450/550 or 450/595 nm can also be used. The plate can also be read at a single wavelength of 450 nm, which will give a somewhat higher reading.
- **(Optional) Software package facilitating data generation and analysis**
- **500 or 1,000 mL graduated cylinder.**
- **Reagent reservoirs**
- **Deionized water of the highest quality**
- **Disposable paper towels**

---

## Precautions and Recommendations

---

- **Although we suggest to conduct experiments as outlined below, the optimal experimental conditions will vary depending on the parameters being investigated, and must be determined by the individual user.**
- **Wear gloves to avoid S100A11 contamination from your skin.**
- Allow all the components to come to room temperature before use.
- All microplate strips that are not immediately required should be returned to the zip-lock pouch, which must be carefully resealed to avoid moisture absorption.
- Do not use kit components beyond the indicated kit expiration date.
- Use only the microtiter wells provided with the kit.
- Rinse all detergent residues from glassware.
- Use deionized water of the highest quality.
- Do not mix reagents from different kits.
- The buffers and reagents in this kit may contain preservatives or other chemicals. Care should be taken to avoid direct contact with these reagents.
- Do not mouth pipette or ingest any of the reagents.
- Do not smoke, eat, or drink when performing the assay or in areas where samples or reagents are handled.
- Dispose of tetra-methylbenzidine (TMB) containing solutions in compliance with local regulations.
- Avoid contact with the acidic Stop Solution and Substrate Solution, which contains hydrogen peroxide.
- Wear gloves and eye protection when handling immunodiagnostic materials and samples of human origin, and these reagents. In case of contact with the Stop Solution and the Substrate Solution, wash skin thoroughly with water and seek medical attention, when necessary.
- **Biological samples may be contaminated with infectious agents. Do not ingest, expose to open wounds or breathe aerosols. Wear protective gloves and dispose of biological samples properly.**
- **CAUTION: Sulfuric Acid is a strong acid. Wear disposable gloves and eye protection when handling Stop Solution.**

---

## Sample Collection and Storage

---

**Serum:** Use a serum separator tube and allow samples to clot for  $60 \pm 30$  minutes. Centrifuge the samples at  $4^{\circ}\text{C}$  for 10 minutes at  $1,000 \times g$ . Remove serum and assay immediately or store samples on ice for up to 6 hours before assaying. Aliquots of serum may also be stored at below  $-70^{\circ}\text{C}$  for extended periods of time. Avoid repeated freeze-thaw cycles.

**Cell culture supernatant:** Remove any particulates by centrifugation and assay immediately or aliquot and store samples at below  $-70^{\circ}\text{C}$ . Avoid repeated freeze-thaw cycles.

**Other biological samples:** MBL has not tested.

(*e.g.* Remove any particulates by centrifugation and assay immediately or aliquot and store samples at below  $-70^{\circ}\text{C}$ . Avoid repeated freeze-thaw cycles. Individual users should determine appropriate conditions when using other types of samples.)

---

## Detailed Protocol

---

The MBL Research Product **CircuLex S100A11 ELISA Kit** is provided with removable strips of wells so the assay can be carried out on separate occasions using only the number of strips required for the particular determination. Since experimental conditions may vary, an aliquot of the human S100A11 Standard within the kit, should be included in each assay as a calibrator. Disposable pipette tips and reagent troughs should be used for all liquid transfers to avoid cross-contamination of reagents or samples.

### Preparation of Working Solutions

All reagents need to be brought to room temperature prior to the assay. Assay reagents are supplied ready-to-use, with the exception of **10X Wash Buffer** and **Human S100A11 Standard**.

1. Prepare a working solution of Wash Buffer by adding 100 mL of the **10X Wash Buffer** to 900 mL of deionized (distilled) water (ddH<sub>2</sub>O). Mix well. Store at 4°C for two weeks or -20°C for long-term storage.
2. Reconstitute **Human S100A11 Standard** with **X\* mL** of ddH<sub>2</sub>O. The concentration of the S100A11 in vial should be **4 ng/mL**, which is referred to as a **Master Standard** of S100A11.

**\*The amount is changed depending on lot. See the real "User's Manual" included in the kit box.**

Prepare Standard Solutions as follows:

Use the **Master Standard** to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The 1,000 pg/mL standard (Std.1) serves as the highest standard. The **Dilution Buffer** serves as the zero standard (Blank).

	Volume of Standard	Dilution Buffer	Concentration
Std.1	150 µL of Master Standard (4 ng/mL)	450 µL	1,000 pg/mL
Std.2	300 µL of Std. 1 (1,000 pg/mL)	300 µL	500 pg/mL
Std.3	300 µL of Std. 2 (500 pg/mL)	300 µL	250 pg/mL
Std.4	300 µL of Std. 3 (250 pg/mL)	300 µL	125 pg/mL
Std.5	300 µL of Std. 4 (125 pg/mL)	300 µL	62.5 pg/mL
Std.6	300 µL of Std. 5 (62.5 pg/mL)	300 µL	31.3 pg/mL
Std.7	300 µL of Std. 6 (31.3 pg/mL)	300 µL	15.6 pg/mL
Blank	-	300 µL	0 pg/mL

**Note:** Do not use a Repeating pipette. Change tips for every dilution. Wet tip with Dilution Buffer before dispensing. Unused portions of Master Standard should be aliquoted and stored at below -70°C immediately. Avoid multiple freeze and thaw cycles.

### Sample Preparation

Dilute samples with **Dilution Buffer**.

- Serum samples may require a 10-20 fold dilution.
- Other biological samples require neat to appropriate dilution. Optimal dilutions of cell conditioned medium for measurement are indicated below;
  - A431 cell culture medium: 200-400 fold dilution
  - HeLa cell culture medium: 30-60 fold dilution
  - LoVo cell culture medium: 30-60 fold dilution

## Assay Procedure

1. Remove the appropriate number of microtiter wells from the foil pouch and place them into the well holder. Return any unused wells to the foil pouch, refold, seal with tape and store at 4°C.
2. Dilute samples with **Dilution Buffer**. (See “Sample Preparation” above.)
3. Pipette **100 µL** of **Standard Solutions (Std1-Std7, Blank)** and the **diluted samples** in duplicates, into the appropriate wells.
4. Incubate the wells **at room temperature (ca.25°C) for 60 minutes, shaking at ca. 300 rpm on an orbital microplate shaker.**
5. Wash 4-times by filling each well with Wash Buffer (350 µL) using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer.
6. Add **100 µL** of **HRP conjugated Detection Antibody** into each well.
7. Incubate the wells **at room temperature (ca.25°C) for 60 minutes, shaking at ca. 300 rpm on an orbital microplate shaker.**
8. Wash 4-times by filling each well with Wash Buffer (350 µL) using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer.
9. Add **100 µL** of **Substrate Reagent** to each well. Avoid exposing the microtiter plate to direct sunlight. Covering the wells with e.g. aluminum foil is recommended. Return Substrate Reagent to 4°C immediately after the necessary volume is removed.
10. Incubate the wells **at room temperature (ca.25°C) for 10-20 minutes, shaking at ca. 300 rpm on an orbital microplate shaker.** (The incubation time may be extended up to 30 minutes if the reaction temperature is below than 20°C).
11. Add **100 µL** of **Stop Solution** to each well in the same order as the previously added Substrate Reagent.
12. Measure absorbance in each well using a spectrophotometric microplate reader at dual wavelengths of 450/540 nm. Dual wavelengths of 450/550 or 450/595 nm can also be used. Read the microplate at 450 nm if only a single wavelength can be used. Wells must be read within 30 minutes of adding the Stop Solution.

**Note-1:** Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.

**Note-2:** Reliable standard curves are obtained when either O.D. values do not exceed 0.25 units for the blank (zero concentration), or 3.0 units for the highest standard concentration.

**Note-3:** If the microplate reader is not capable of reading absorbance greater than the absorbance of the highest standard, perform a second reading at 405 nm. A new standard curve, constructed using the values measured at 405 nm, is used to determine S100A11 concentration of off-scale samples. The readings at 405 nm should not replace the on-scale readings at 450 nm.

---

## Calculations

---

Average the duplicate readings for each Standard Solution, control, and sample and subtract the average zero standard optical density. Plot the optical density for the standards versus the concentration of the standards and draw the best curve. The data can be linearized by using log/log paper and regression analysis may be applied to the log transformation. To determine the human S100A11 concentration of each sample, first find the absorbance value on the y-axis and extend a horizontal line to the standard curve. At the point of intersection, extend a vertical line to the x-axis and read the corresponding human S100A11 concentration. If the samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

1. The dose-response curve of this assay fits best to a sigmoidal four-parameter logistic equation. The results of unknown samples can be calculated with any computer program having a four-parameter logistic function. It is important to make an appropriate mathematical adjustment to accommodate for the dilution factor.
2. Most microtiter plate readers perform automatic calculations of analyte concentration. The calibration curve is constructed by plotting the absorbance (Y) of calibrators versus log of the known concentration (X) of calibrators, using the four-parameter function. Alternatively, the logit log function can be used to linearize the calibration curve (i.e. logit of absorbance (Y) is plotted versus log of the known concentration (X) of calibrators).

---

## Measurement Range

---

The measurement range is 15.6 pg/mL to 1,000 pg/mL. Any sample reading higher than the highest standard should be diluted with Dilution Buffer in higher dilution and re-assayed. Dilution factors need to be taken into consideration in calculating the human S100A11 concentration.

---

## Troubleshooting

---

1. All samples and controls should be assayed in duplicate, using the protocol described in the **Detailed Protocol**. Incubation times or temperatures significantly different from those specified may give erroneous results.
2. Poor duplicates, accompanied by elevated values for wells containing no sample, indicate insufficient washing. If all instructions in the **Detailed Protocol** were followed accurately, such results indicate a need for washer maintenance.
3. Overall low signal may indicate that desiccation of the plate has occurred between the final wash and addition of Substrate Reagent. Do not allow the plate to dry out. Add Substrate Reagent immediately after wash.

---

## Reagent Stability

---

All of the reagents included in the MBL Research Product **CircuLex S100A11 ELISA Kit** have been tested for stability. Reagents should not be used beyond the stated expiration date. Upon receipt, kit reagents should be stored at 4°C, except the reconstituted S100A11 Standard must be stored at below -70°C. The Microplate should be stored in the original foil bag sealed by the zip lock and containing a desiccant pack.

---

## Assay Characteristics


---

### 1. Sensitivity

The limit of detection (defined as such a concentration of human S100A11 giving absorbance higher than mean absorbance of blank\* plus three standard deviations of the absorbance of blank: A blank + 3SD blank) is better than 4.34 pg/mL of sample.

\* Dilution Buffer was pipetted into blank wells.

### Typical Standard Curve

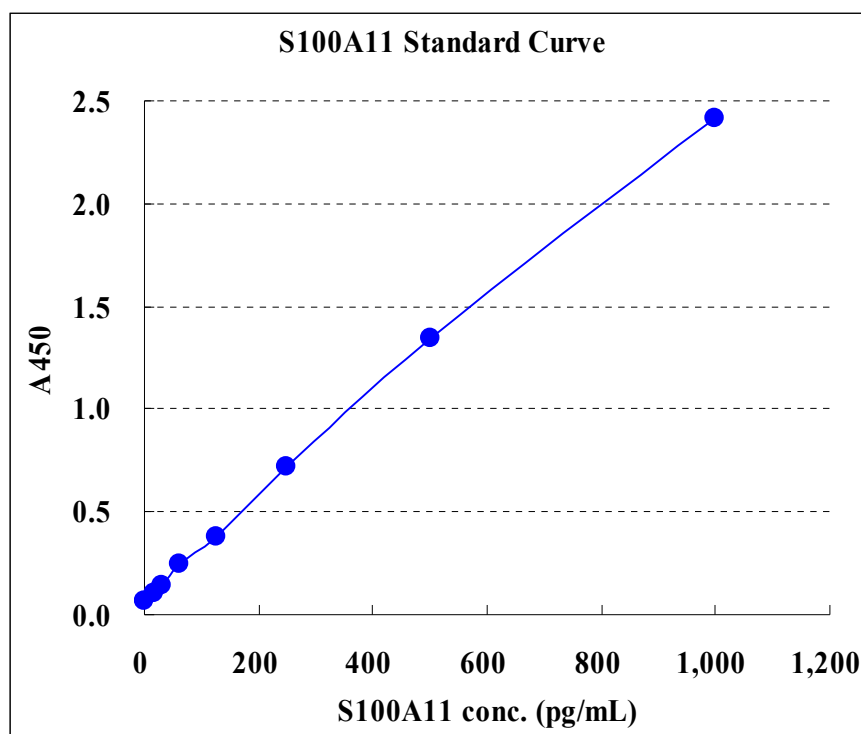

## 2. Precision

### Intra-assay Precision (Precision within an assay)

Three samples of known concentration were tested sixteen times on one plate to assess intra-assay precision.

- Intra-assay (Within-Run, n=16) CV=2.1-3.2 %

S100A11 conc. (pg/ml)			
	Sample 1	Sample 2	Sample 3
1	78.7	169.5	337.8
2	85.4	168.9	359.0
3	90.4	174.5	357.2
4	85.9	176.4	369.6
5	87.9	178.4	360.8
6	83.2	174.7	363.4
7	82.1	179.0	355.9
8	83.5	181.0	360.4
9	83.1	172.5	338.3
10	86.5	170.5	353.1
11	87.8	170.9	363.6
12	86.6	175.7	359.4
13	86.0	170.9	359.6
14	85.2	171.8	358.0
15	83.6	174.6	356.3
16	84.3	176.5	363.3
<b>MAX.</b>	<b>90.4</b>	<b>181.0</b>	<b>369.6</b>
<b>MIN.</b>	<b>78.7</b>	<b>168.9</b>	<b>337.8</b>
<b>MEAN</b>	<b>85.0</b>	<b>174.1</b>	<b>357.2</b>
<b>S.D.</b>	<b>2.72</b>	<b>3.60</b>	<b>8.41</b>
<b>C.V.</b>	<b>3.2%</b>	<b>2.1%</b>	<b>2.4%</b>

Inter-assay Precision (Precision between assays)


Three samples of known concentration were tested in five separate assays to assess inter-assay precision.

- Inter-assay (Run-to-Run, n=5) CV=6.3-10.7 %

	S100A11 conc. (pg/ml)		
	Sample 1	Sample 2	Sample 3
1	90.7	185.6	345.5
2	112.2	205.6	407.8
3	89.4	196.6	426.6
4	94.4	206.8	466.0
5	86.9	178.7	414.2
<b>MAX.</b>	<b>112.2</b>	<b>206.8</b>	<b>466.0</b>
<b>MIN.</b>	<b>86.9</b>	<b>178.7</b>	<b>345.5</b>
<b>MEAN</b>	<b>94.7</b>	<b>194.7</b>	<b>412.0</b>
<b>S.D.</b>	<b>10.2</b>	<b>12.3</b>	<b>43.5</b>
<b>C.V.</b>	<b>10.7%</b>	<b>6.3%</b>	<b>10.6%</b>

**3. Linearity**

Two samples were diluted with Dilution Buffer and assayed after dilution. The neat sample was set to 1. Please note that all samples including the neat sample were 8-fold diluted as stated in the Assay Procedure. The results are summarized in the figure below.

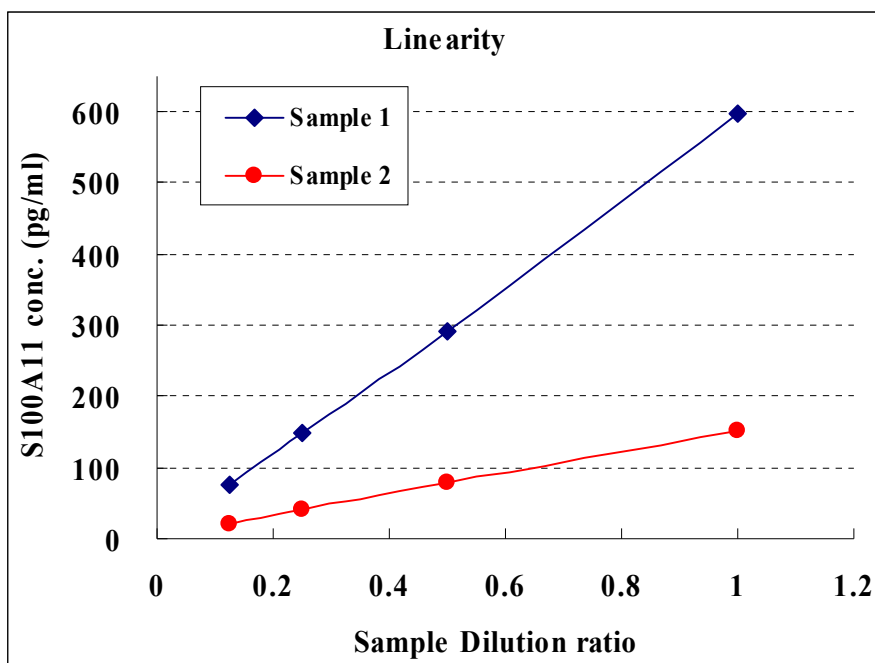

## Example of Test Results

Fig.1 S100A11 Level in conditioned media of several cell lines

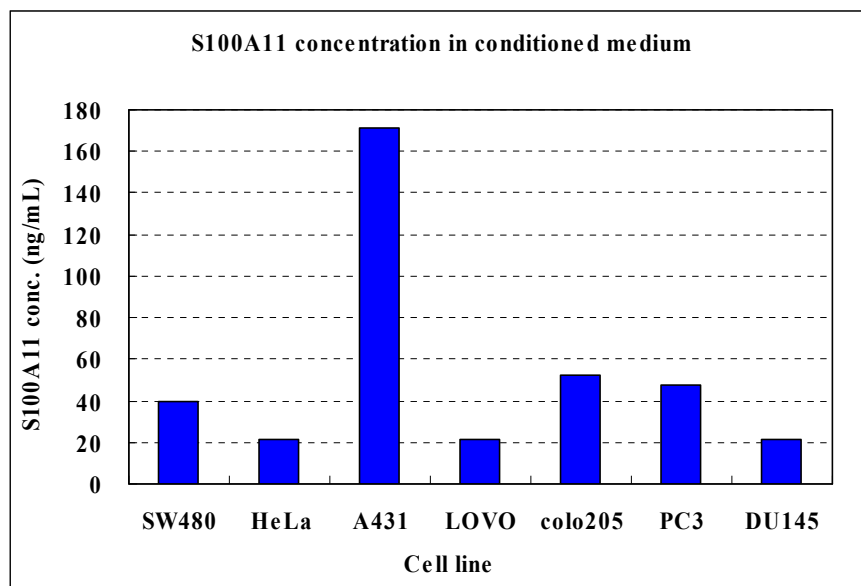


Fig.2 S100A11 concentration in cell lysates (ca. 1 mg/mL protein concentration) from many cell lines


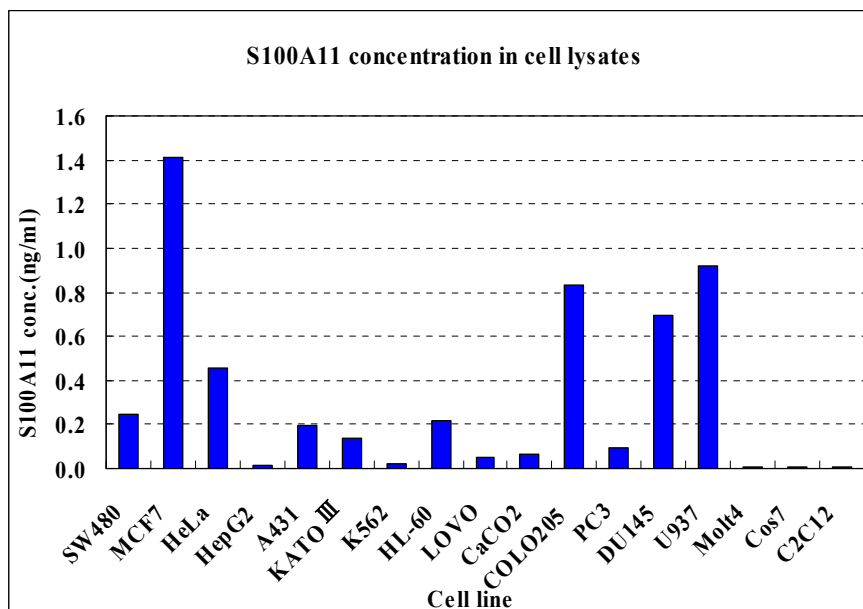


Fig.3 Serum S100A11 level in 20 CRP-positive volunteers and 20 healthy volunteers.

Average S100A11 concentration in sera

CRP-positive volunteers: 1,091.6 pg/mL (n=20)

Healthy volunteers: 526.3 pg/mL (n=20)

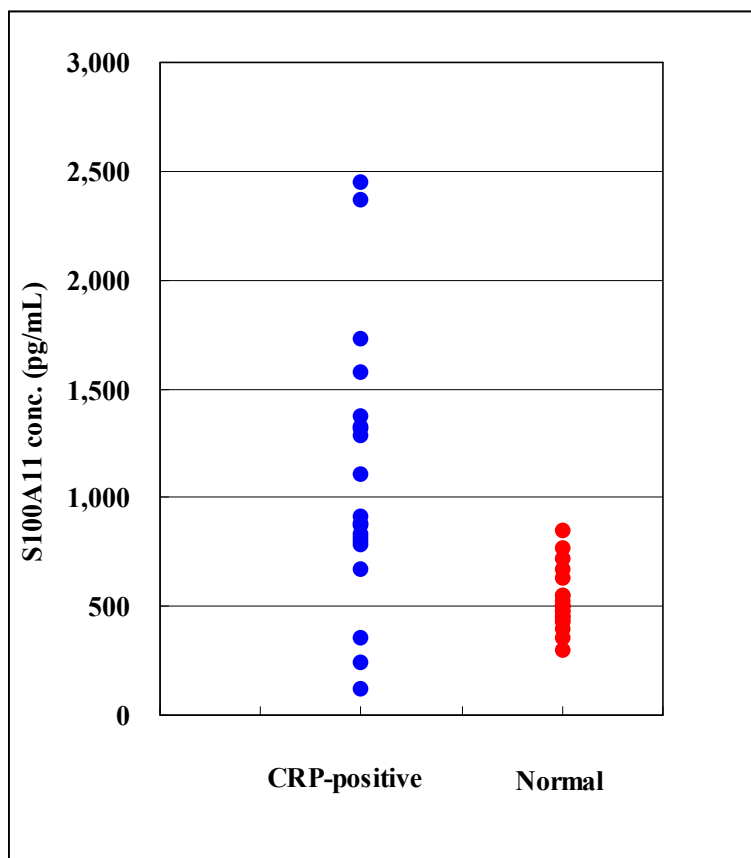

---

## References

---

1. Todoroki H, Kobayashi R, Watanabe M, Minami H, Hidaka H.; Purification, characterization, and partial sequence analysis of a newly identified EF-hand type 13-kDa Ca<sup>2+</sup>-binding protein from smooth muscle and non-muscle tissues. *J Biol Chem* 266: 18668-18673, 1991
2. Ohta H, Sasaki T, Naka M, Hiraoka O, Miyamoto C, Furuichi Y, Tanaka T.; Molecular cloning and expression of the cDNA coding for a new member of the S100 protein family from porcine cardiac muscle. *FEBS Lett* 295: 93-96, 1991
3. Rety S, Osterloh D, Arie JP, Tabaries S, Seemann J, Russo-Marie F, Gerke V, Lewit-Bentley A.; Structural basis of the Ca<sup>2+</sup>-dependent association between S100C (S100A11) and its target, the N-terminal part of annexin I. *Structure* 8: 175-184, 2000
4. Ning Chang, Cindy Sutherland, Eva Hesse, Robert Winkfein, William B. Wiehler, Mark Pho, Claude Veillette, Susan Li, David P. Wilson, Eniko Kiss, and Michael P. Walsh.; Identification of a novel interaction between the Ca<sup>2+</sup>-binding protein S100A11 and the Ca<sup>2+</sup>-and phospholipid-binding protein annexin A6. *Am J Physiol Cell Physiol* 292: C1417-C1430, 2007
5. Zhao XQ, Naka M, Muneyuki M, Tanaka T.; Ca<sup>2+</sup>-dependent inhibition of actin-activated myosin ATPase activity by S100C (S100A11), a novel member of the S100 protein family. *Biochem Biophys Res Commun* 267: 77-79, 2000.
6. Ruse M, Lambert A, Robinson N, Ryan D, Shon KJ, Eckert RL.; S100A7, S100A10, and S100A11 are transglutaminase substrates. *Biochemistry* 40: 3167-3173, 2001.
7. Deloulme JC, Assard N, Mbele GO, Mangin C, Kuwano R, Baudier J.; S100A6 and S100A11 are specific targets of the calcium- and zinc-binding S100B protein in vivo. *J Biol Chem* 275: 35302-35310, 2000.
8. Sakaguchi M., Sonogawa H., Nukui T., Sakaguchi Y., Miyazaki M., Namba M., Huh N. H. ; Bifurcated converging pathways for high Ca<sup>2+</sup>- and TGFbeta-induced inhibition of growth of normal human keratinocytes. *Proc. Natl. Acad. Sci. USA* 102: 13921-13926, 2005
9. Sakaguchi M., Miyazaki M., Takaishi M., Sakaguchi Y., Makino E., Kataoka N., Yamada H., Namba M., Huh N. H.; S100C/A11 is a key mediator of Ca(2+)-induced growth inhibition of human epidermal keratinocytes. *J. Cell Biol* 163: 825-835, 2003

For more information, please visit our website at

<https://ruo.mbl.co.jp/>.

### MANUFACTURED BY

 **MBL MEDICAL & BIOLOGICAL LABORATORIES CO., LTD.**

URL: <https://ruo.mbl.co.jp>

E-mail: [support@mbl.co.jp](mailto:support@mbl.co.jp)

CycLex/CircuLex products are supplied for research use only. CycLex/CircuLex products and components thereof may not be resold, modified for resale, or used to manufacture commercial products without prior written approval from MBL. To inquire about licensing for such commercial use, please contact us via email.